

Test Report

No.: T32020260466SN

Date: JUL 14, 2020

Page 2 of 3

Bacterial filtration efficiency (BFE) (EN14683:2019+AC:2019 Appendix B)

Test Side : White Colour (Inside)
 Pre-Conditioning : Minimum of 4 hours at 21±5°C and 85±5% R.H.
 Test Condition : 21±2 °C and 30-50% R.H.
 Dimensions of test specimen : 157 mm x 204 mm
 BFE Test Area : 49 cm²
 BFE Flow Rate : 28.3 l/min
 Test bacteria : Staphylococcus aureus ATCC 6538
 Positive Control Average : 2.9 x 10³ CFU
 Negative Monitor Count : < 1 CFU

AOP-KF Mask (Brand New)

Test Specimen	Percent BFE (%)
1	99.9
2	99.9
3	99.9
4	99.9
5	99.9


AOP-KF Mask (Used for 7 Days)

Test Specimen	Percent BFE (%)
1	99.9
2	99.9
3	99.9
4	99.9
5	99.9

This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Photo Appendix

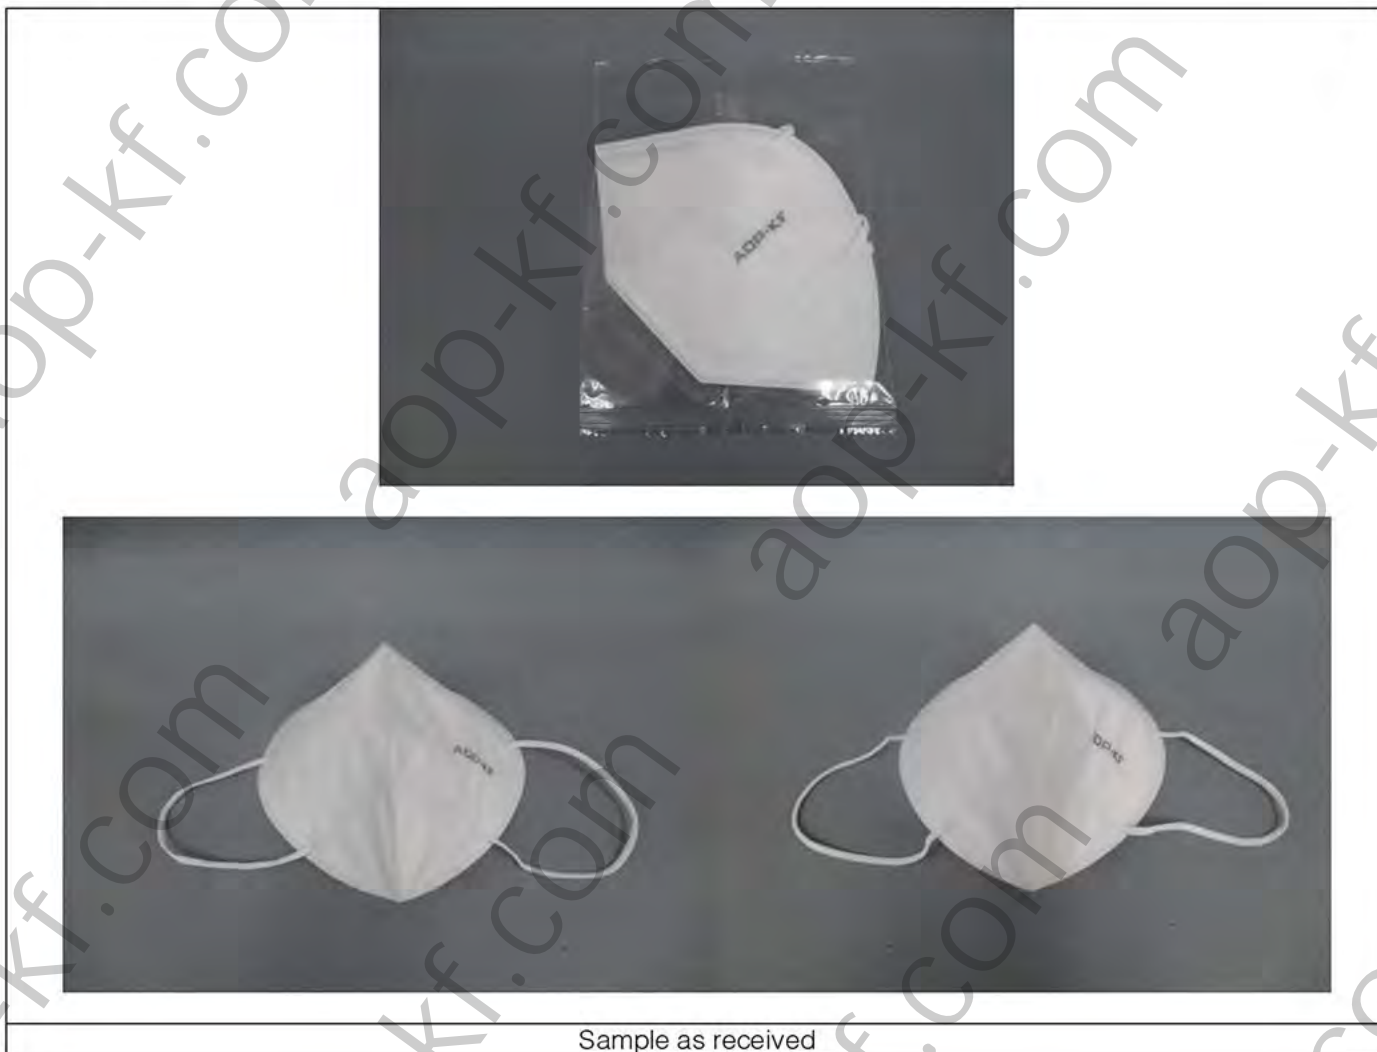

Sample as received

*** End of Report ***

This document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.